

# VRI4 – Manual



## VRI 4.0 includes the following features:

- 12 Dials
- Base 10, Base 12, Base 336 and Base 44 capability
- Potentiating up to X45 (D45)
- Witness can be by letters (e.g. name) or by a picture
- Flexible Broadcast-timer
- Extendable Ratebook, with basic Ratebook built in
- Extendable list of recipes, with basic recipe list built in
- Direct mode and programmable mode for performing a timed list of broadcasts
- Up- and download possibility for list of broadcasts
- Creation of broadcasts from Ratebook, recipes or by free input possible
- After download and installation, the VRI4 can be run without internet connection

Download address v4.0: <https://brave-glacier-087932403.5.azurestaticapps.net/>

Download address v4.1 (incl. Analysis): <https://virtual-radionics.com/VRI4/>

Email contact: [Geoffrey.Ardens@gmail.com](mailto:Geoffrey.Ardens@gmail.com)

**Important - Please note:**

Radionics is a method of sending precisely defined healing energy to people, animals or plants, no matter where they are in the world. The name reflects the view of early practitioners that they were 'broadcasting' healing, but we now believe that radionic treatment occurs at a level of reality (no comma) beyond 3-dimensional space where there is no distance between us. This is a challenging concept, but it is entirely compatible with modern physics and also with the ancient mystic teaching that at some level we are all one, and that at this level exchanges of healing energy can occur.

Radionics is classified as a complementary therapy, that is it should be used as a supplement to conventional medical care, not as a substitute for it. Experience indicates that radionics can help to speed recovery from illness and to maintain us in good health.

The manual delivered with the Instrument describes how to use the Virtual Radionic Instrument. In order to use it effectively it is essential to have received training in radionic methods first. If you are not a trained radionic practitioner you are strongly advised to take a course in radionics to understand how it works and how to work with it.


You can obtain details from The Radionic Association The Radionic Association, Baerlein House, Goose Green, Deddington, Banbury, Oxon. OX15 0SZ UK (01869) 338852 | Outside UK +44 1869 338852  
[enquiries@radionic.co.uk](mailto:enquiries@radionic.co.uk)

## Installation


In your browser (e.g., Chrome, Safari, etc.) go to [vri4.000webhostapp.com](https://vri4.000webhostapp.com) or <https://brave-glacier-087932403.5.azurestaticapps.net/> to open the VRI4 application. The VRI4 will appear in your browser window after all data have been loaded into your browser cache (0 – 100% progress circle).

You can now use the VRI4 already, however before installation it will only run if an internet connection is available. To make it independent from internet, you need to click on the installation button, which is displayed on the right-hand side of your address bar.

In Chrome browser you see this screen symbol with an arrow.




In Microsoft Browser, it is an icon with + sign



When you hover over this sign with your mouse, a pop up is indicating, that you can install the VRI4 on your device. With a click on this icon, you start the installation process. Please follow the instructions. You can decide whether you want to have an icon for the VRI4 set on your Taskbar (optional).

After installation the VRI4 runs without internet connection when started from the created Desktop-icon. The VRI4 will appear in a separate window, outside of the regular browser.

With using the three dots, you can again deinstall the VRI4, if required.

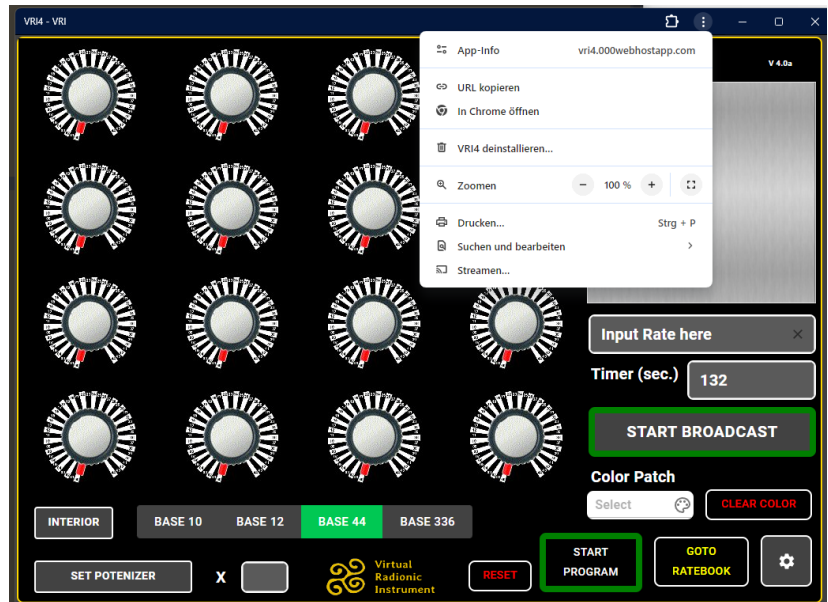


On **Android** devices you may look into the settings menu of the Browser to find an entry called "Installation" with allows you to install the web app on the device and put an icon to the screen of your device.

**Please be cautious with clearing the Browser Cache**, as this will also erase the cached files for VRI4 and you need to re-download the VRI4 to run it again. Also, all data stored in the browser (broadcast lists, pictures, any uploaded ratebook and recipe data) will be erased by clearing the browser cache.

If you need to clear the cache for any reason, you should in beforehand download all important data and upload them again, after you have cleared the browser cache.

## Basic use – Instant broadcast

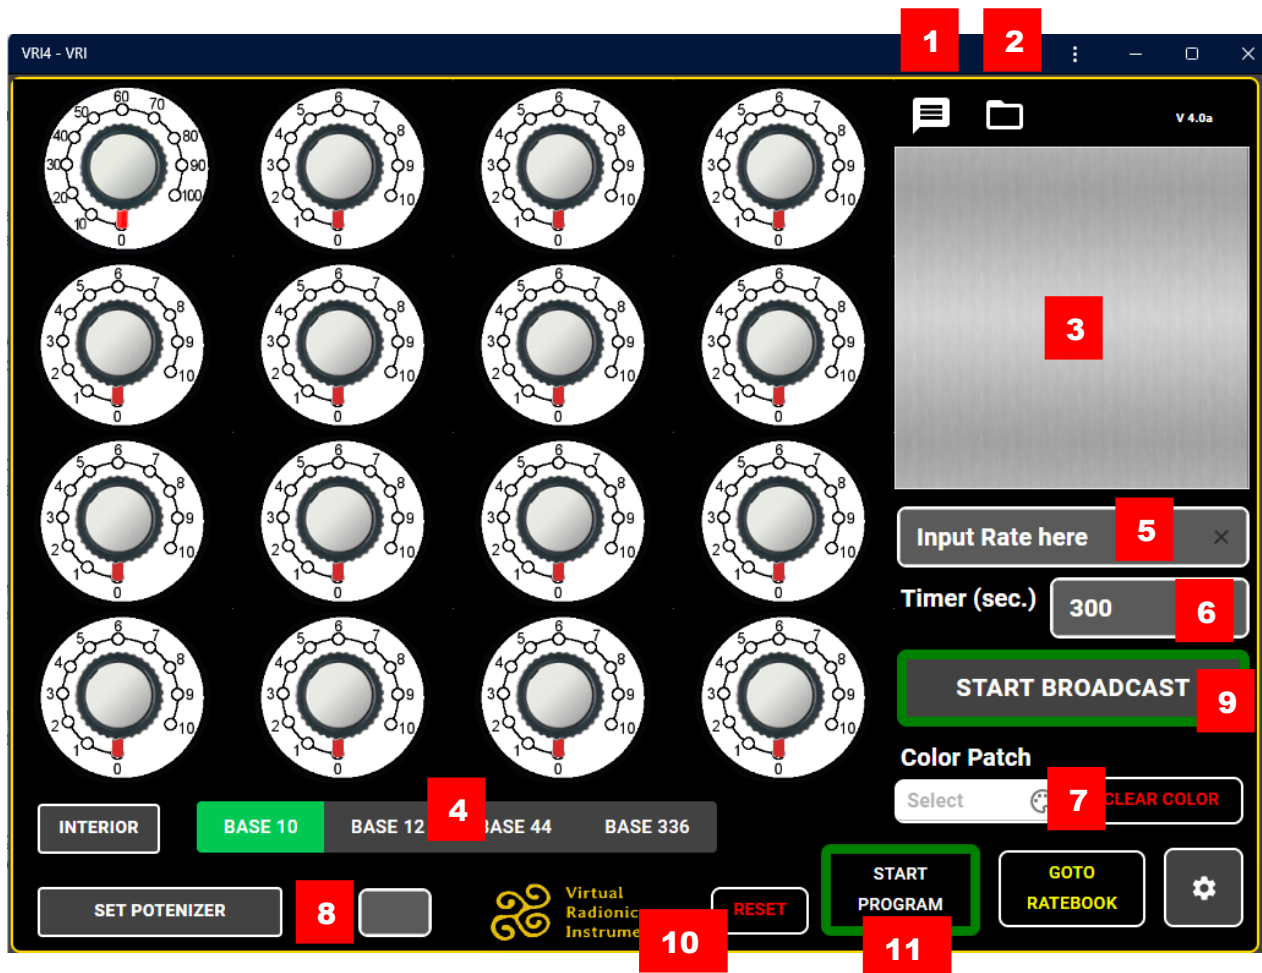

- ❶ With click on this Symbol an empty witness is created on the well. You can click into this field and enter e.g. a name, for whom this broadcast is intended. To hide the witness, you click on the icon again. The Icon is red when a witness is displayed
- ❷ Clicking on this icon you can choose a picture from your device, which is then displayed on the well and can be used for broadcast. The icon turns red. Clicking again on the icon will hide the picture and reset the icon to white color
- ❸ Representation of the well. The energy of the instrument is emitted there. You can place any witness or any flask for remedy making on here
- ❹ With these buttons you can choose the Base you want to use for your broadcast. Base10, Base12, Base 44 and Base 336 is possible. The outline of the dials will be changed accordingly (both front panel and interior)

- 5 You can input a rate in this field using your keyboard. **The rate is only set when you press ENTER.** It is important to stick to the nomenclature of correctly writing the rates. Base 44 rates need to be written with spaces in between the dial settings – e.g. 12 34 12 33
- 6 In this field you can enter the broadcast time in seconds. Standard times are 300 s (5 min) for Base 10 / 12 / 336 / Peggotty and 132 s (2.2 min) for Base 44.
- 7 If you want to add a color to your broadcast you can click here. A color palette is displayed, where you can select a color. If you need a larger variety of colors you can change the palette by
  - 1.) click on 7 to display the color palette
  - 2.) make a double click – the palette is changing to a more complex pattern
  - 3.) select a color or, if still not complex enough, make another double click with displayed palette and double click you can switch between the different palettes.
- 8 Here you can type in a potency and set the potentizer. Potencies of X1–45 are possible (D1 – D45).
- 9 To start a Broadcast you click on the “Start Broadcast” button. The outline will change to “Stop Broadcast” and the broadcast will be started. You can see the timer running and when using the interior button you can see the dials being connected to the well during the broadcast. The broadcast will stop automatically after the timer has reached 0 s.
- 10 The reset button can be used to bring the instrument back into a standard condition
- 11 With the START PROGRAM button you start the broadcast from the broadcast list. The VRI4 will look in the broadcast list whether a broadcast is scheduled for the given time, or whether a forecast is already waiting to be performed. The VRI will take the next broadcast from the list and will continue until no broadcast is scheduled anymore for current or past time, but only for future time. The well will then show the date and time of the next scheduled forecast. You can also click into the witness field and scroll down to see how many broadcasts are still left in schedule. During program mode, the other buttons are locked. You need first stop the program mode to be able to work with the VRI4 again.

The remaining buttons on the lower right are related to access the built in ratebook and recipe-list, as well as to settings part, where up- and download of lists are possible. Those will be explained in the next chapters.

With the INT(erior) button on the left side you can look inside the Black Box. In the interior screen, there is only one button, which you can use to switch back to the front panel.

## Ratebook – Creating Forecast lists

When clicking on “GOTO RATEBOOK” the ratebook page is opened.

On this page you can create broadcasts using the built in ratebook.

You also can pick broadcast from the recipe list for frequent ailments, or you can freely create broadcasts of you own by using a simple form.



The screenshot shows the VR14 Ratebook interface with the following numbered callouts:

- 1**: Select a name dropdown menu.
- 2**: ADD button.
- 3**: Select a Category dropdown menu.
- 4**: X button to clear a line.
- 5**: Potency (X or D max. D45) input field.
- 6**: ADD TO LIST button.
- 7**: CLEAR LIST button.
- 8**: INPUT FORM button.
- 9**: STORE LIST FOR BROADCAST button.

Date	Name	Base	Desc1	Rate1	Rate2	Desc2	Potency	Duration	Color	Repetitions	Pause
[Empty table body]											

- 1 In this field you can select the name or description you want to use for the Broadcast. Initially there is nothing to be selected, therefore you have to first ADD names or descriptions to the list. With upload of pictures in the Settings page, the name entry is created automatically in this list (see Settings page description)
- 2 Clicking on ADD will activate the “Select a name” field for text input. You can now type in a name or description. The ADD field transforms into CONFIRM. Clicking on CONFIRM will take the name/description you have typed in into the list, so you can select it in future. The REMOVE button will remove the selected name from the list.
- 3 This box will help you to select an appropriate rate for your broadcast. You can subsequently select for both lines a category and item and a rate. E.g. “Organs” -> Visual -> Base 10 : 31591 You can use one or both lines to create broadcasts.
- 4 You can clear the lines individually by clicking on the “X” button
- 5 In this row you can enter data for the potency you want to use, the duration of the broadcast the intended number of repetitions, the pause between the broadcasts and a color patch used for the broadcasts. If you leave the fields blank, the standard settings taken for the broadcast are:  
Potency: 0  
Duration: 5 min Base10/12/336/Peggotty, 2.2 min Base 44

Repetitions: 1  
Pause: 1  
Color: white/none


Repetitions: 1 means that the broadcast is done once. With only one performance the Pause is obsolete and has not meaning.

- 6 If you have created the intended single broadcast by filling the lines, you can add this broadcast to the list for Broadcasts by clicking "ADD TO LIST". The Broadcast information will then appear in the list below.

PLEASE BE AWARE THAT ONLY THOSE BROADCASTS FROM THE LIST ARE TRANSFERRED TO THE BROADCAST-LIST" USED FOR PROGRAMMED BROADCAST, WHICH HAVE BEEN FINALLY STORED BY CLICKING ON THE GREEN "STORE LIST FOR BROADCAST"!

- 7 This list is collecting the broadcasts you have created. The broadcasts are only temporary stored in this list and will be deleted when leaving the page (going back to HOME). To store this list into the Broadcastlist used for program mode you need to click on the "STORE LIST FOR BROADCAST". By this the list is emptied and the broadcasts are transferred into the internal Broadcastlist.

- 8 In case you want to enter broadcasts not available via ratebook or recipe-list, you can enter your data using a form, which pops up when clicking on "INPUT FORM". With ACCEPT the data are put into the list, with CANCEL the form will be closed without taking a broadcast to the list.

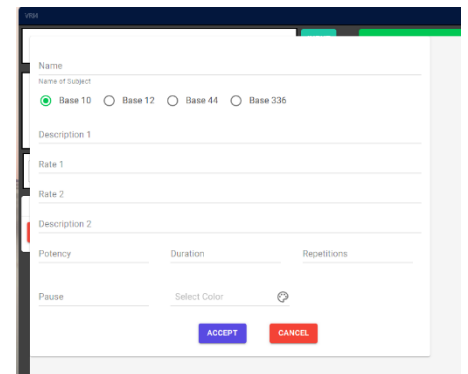A screenshot of a web form for creating a broadcast. The form has a title bar with a close button. It contains several input fields: 'Name of Subject' with radio buttons for 'Base 10', 'Base 12', 'Base 44', and 'Base 336'; 'Description 1'; 'Rate 1'; 'Rate 2'; 'Description 2'; 'Potency'; 'Duration'; 'Repetitions'; 'Pause'; and 'Select Color' with a color picker icon. At the bottom, there are two buttons: 'ACCEPT' (blue) and 'CANCEL' (red).


- 9 VERY IMPORTANT! To transfer and add the created list of broadcasts into the internal storage for programmed broadcasts, you need to click on "STORE LIST FOR BROADCAST". By this the list of broadcasts you have created are stored and list on the page is emptied. Now you can return to the HOME page by clicking on the "HOME" button.

If you leave the page without "STORE LIST FOR BROADCAST", another pop-up window will appear, give you the chance to store the created broadcasts. If you skip this, the created list of broadcasts will be erased with leaving the page.

## Recipe – List

In the drop down list of the first category you find an entry named "...Recipes..."

Clicking on this item, a second drop down list is opened where you can choose from a list of areas of common ailments. Choosing an area opens a drop list where you choose from a list of common ailments. With clicking on "ADD" you can add the recommended broadcasts for this condition into the temporary broadcast list on the page. With "CANCEL" you can return to the standard selection view again, without selecting any broadcast recipe.

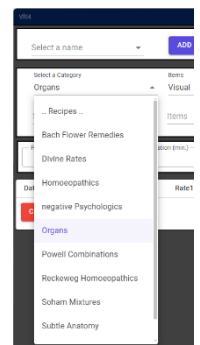

## **HOME**

With clicking on “HOME” you return to the instrument’s front panel page.

You now can start (or continue) with your broadcasts by clicking on “START PROGRAM”. While a program is running, all buttons are blocked, except the “STOP PROGRAM”.




## Settings – list management

This page is mainly for managing list, which can be used in VRI4 and enable the download the list content stored in the instrument, but also the upload of customized list e.g. to extend the ratebook, to add recipes to the recipe list and to manage or work on the broadcastlist outside the VRI4.



### Line 1: UPLOAD PICTURES, Instrument Settings Backup and Restore, and Language Settings for Analysis page.

This button let you upload pictures which can be used in program mode. The pictures are automatically laid on the well with broadcasts. With upload of the picture, the filename will be transferred into the name list. Therefore, you may choose the filenames for the pictures appropriately e.g. Firstname\_Lastname.jpg

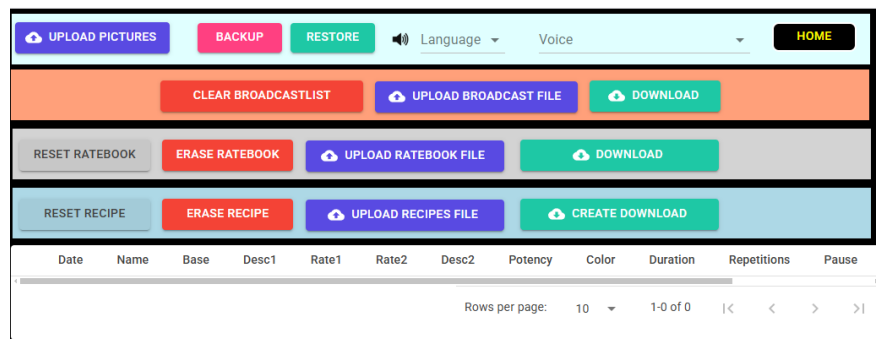

The pictures will also be displayed in the Ratebook page to facilitate the selection

### Backup and Restore

With Backup, the total status of your instrument, including the local storage is saved. This includes the Broadcast list, Ratebook, Recipe-list, uploaded pictures and names list.

In case you need to erase your browser cache (e.g. with potential updates) you need to click on BACKUP first. A file is downloaded for you with looks like VRI4\_localStorageData\_20240629\_111923.json (VRI4\_localStorageData\_{YYYYMMDD}\_{hhmmss}.json).

Now you can erase your browser cache.

To restore your instrument, you click on RESTORE and select your downloaded .json file. You may need to restart your browser after restoring.

You also can transport a VRI4 status from one device to another (e.g. transport the status of the VRI4 on your PC to the one on your Android tablet)

### Language Settings for Analysis page

Here you can select the language and speaker who will tell you what to dowse for in Analysis page. This feature is still experimental and depends on the specific installation you have with your PC or your tablet.

### HOME

With "HOME" you can go back to the front panel view of the VRI4 instrument.

## Line2: BROADCASTLIST

You can clear the existing broadcast list in the instrument with “CLEAR BROADCASTLIST”. All broadcasts for program mode stored in the VRI4 will then be cleared.

If you have created a broadcast list outside the VRI4 you can add these broadcasts to the VRI4 broadcast list with “UPLOAD BROADCAST FILE”. If you want to overwrite any existing broadcast list, please click on “CLEAR BROADCASTLIST” first and then upload your file.


With clicking on “DOWNLOAD” a download link is created, from where you can download the internal stored broadcast list. Downloading this list is also helpful to get a template for a broadcast list if you want to create a broadcast list outside the VRI4.

The downloaded list is in .csv format and comma delimited. The text file looks like this

```
"Date","Name","Base","Desc1","Rate1","Rate2","Desc2","Potency","Color","Duration","Repetitions","Pause","Status","last","next"
"29.06.2024 10:14:22","Mark Smith","Base44","","24 44 05 01 14 33 23 43","","","0","yellow","2.2","9","1","",""
"29.06.2024 10:14:22","Mark Smith","Base44","","13 04 11 44","","","0","yellow","2.2","1","1","",""
"29.06.2024 10:14:22","Mark Smith","Base44","","19 21 36 23","","","0","yellow","2.2","4","3","",""
"29.06.2024 10:14:22","Mark Smith","Base336","","34896","","","0","cyan","5","5","4","",""
```

To work on Broadcast files (same for ratebook or recipe files) it is more convenient to import or open those with a spreadsheet program like Excel, OpenOffice Calc, Google sheets or similar program.

You may need to set the delimiter to comma (,) and the text qualifier to quote (") to correctly import the text.

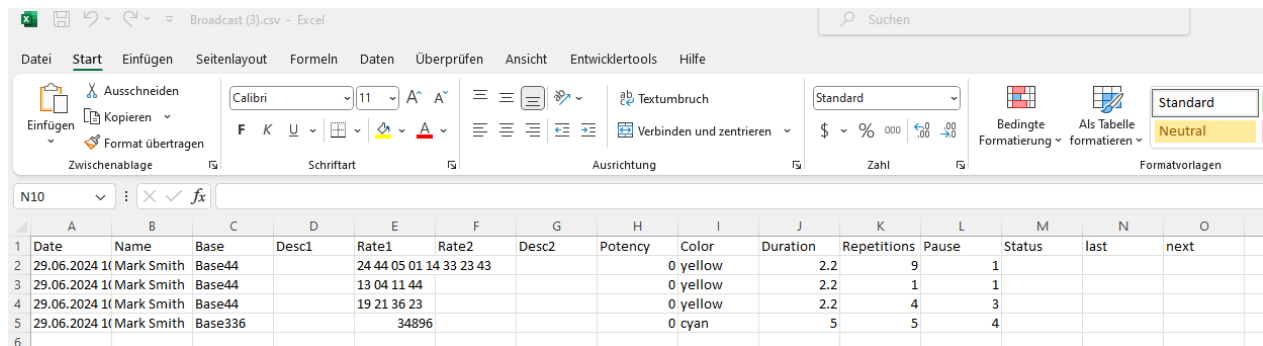

Date	Name	Base	Desc1	Rate1	Rate2	Desc2	Potency	Color	Duration	Repetitions	Pause	Status	last	next
29.06.2024 10:14:22	Mark Smith	Base44		24 44 05 01 14 33 23 43			0	yellow	2.2	9	1			
29.06.2024 10:14:22	Mark Smith	Base44		13 04 11 44			0	yellow	2.2	1	1			
29.06.2024 10:14:22	Mark Smith	Base44		19 21 36 23			0	yellow	2.2	4	3			
29.06.2024 10:14:22	Mark Smith	Base336		34896			0	cyan	5	5	4			

You can now add lines and with your broadcast information. The Desc1 / Desc2 fields are deliberate and may only serve your documentation. You need to add at least Date, Name, Base and Rate1. For blank fields the standard settings will be filled in.

In color field you can use the # values, which however are a bit inconvenient to write and to remember. Therefore, the VRI4 understands a variety of colors in clear names by default. These are:

```

"red" {"#FF0000"}
"green" {"#00FF00"}
"blue" {"#0000FF"}
"yellow" {"#FFFF00"}
"cyan" {"#00FFFF"}
"magenta" {"#FF00FF"}
"black" {"#000000"}
"white" {"#FFFFFF"}
"gray" {"#808080"}
"silver" {"#C0C0C0"}
"maroon" {"#800000"}
"olive" {"#808000"}
"navy" {"#000080"}
"purple" {"#800080"}
"teal" {"#008080"}
"orange" {"#FFA500"}
"violet" {"#8F00FF"}
"purple" {"#800080"}
"cyan" {"#00FFFF"}
"light blue" {"#ADD8E6"}

```



**Line3: RATEBOOK**

These buttons work similar to those in the Broadcast line, with erasing the internal data, and up- and download functions. In addition, you can reset the Ratebook and the recipe-list to their initial settings which are included in the VRI4.

The ratebook file format is as below (Quotes are not mandatory):

```

Category,Item,Base44,Base10,Base336,Base12,Peggotty
Bach Flower Remedies,Agrimony,24 44 29 01,7643,2247,,
Bach Flower Remedies,Aspen,24 44 20 01,3639,4178,,
Soham Mixtures,Immunity 200,05 16 19 25,1456,99112,,
Soham Mixtures,Infection 200,12 18 27 28,3467,48993,,
Soham Mixtures,Injury 30,28 31 32 38,7789,83586,,
Soham Mixtures,Kidney 30,31 33 40 41,88910,13814,,
Skeletal Conditions,Sacro-iliac disease,,,,,40.2854374
Skeletal Conditions,Nerve trunk pressure,,,,,50.11109279
Skeletal Conditions,Cervical rib,,,,,70.74694542

```

	A	B	C	D	E	F	G	H
1	Category	Item	Base44	Base10	Base336	Base12	Peggotty	
2	Bach Flower	Agrimony	24 44 29 01	7643	2247			
3	Bach Flower	Aspen	24 44 20 01	3639	4178			
4	Soham Mixtu	Immunity 20	05 16 19 25	1456	99112			
5	Soham Mixtu	Infection 20	12 18 27 28	3467	48993			
6	Soham Mixtu	Injury 30	28 31 32 38	7789	83586			
7	Soham Mixtu	Kidney 30	31 33 40 41	88910	13814			
8	Skeletal Con	Sacro-iliac disease					40.2854374	
9	Skeletal Con	Nerve trunk pressure					50.1110928	
10	Skeletal Con	Cervical rib					70.7469454	
11								

You can add / change lines and rates as required and store the file again as \*.csv file (comma delimited). Then you can click on upload ratebook and select your new file. This file is then uploaded and the new ratebook is stored in the Browser Cache and is available to the VRI4.

Please keep your personal ratebooks as csv file, because with clearing the browser cache the ratebook will be erased – so it’s good to have a backup!

**Line4: Recipe-list**

The recipe list works similar to the Ratebook. You can download the file as csv with the below structure:

	A	B	C	D	E	F	G	H	I	J	K	L
1	Disease_Category	Disease	Base	Desc1	Rate1	Rate2	Desc2	Potency	Color	Duration	Repetitions	Pause
2	Allergies	seasonal rhinitis	Base10		396	396			0 red		8	5
3	Allergies	seasonal rhinitis	Base336		7671				6 white		10	4
4	Allergies	seasonal rhinitis	Base336		3406				6 white		10	4
5	Allergies	seasonal rhinitis	Base10		40677				0 blue		10	2
6	Allergies	seasonal rhinitis	Base44		07 02 01 20				0 violet		1	1
7	Allergies	seasonal rhinitis	Base10		70.57				0 yellow		7	5
8	Allergies	seasonal rhinitis	Base10		944				0 yellow		10	4
9	Allergies	seasonal rhinitis	Base336		44695				0 white		2	1
10	Allergies	asthmatic attack	Base44		08 43 33 20				0 blue		3	1
11	Allergies	asthmatic attack	Base44		11 37 05 37 29 38 42 41				0 yellow		2	1
12	Allergies	asthmatic attack	Base336		30755				0 Blue		1	1
13	Allergies	asthmatic attack	Base55		24 44 24 21				0 white		2	1
14	Allergies	asthmatic attack	Base10		396	396			0 red		8	5
15	Allergies	allergic reaction to insetct sting	Base44		5612				0 white		6	1
16	Allergies	allergic reaction to insetct sting	Base336		15254				0 violet		4	2
17	Allergies	allergic reaction to insetct sting	Base336		78124				0 green		4	5
18	Allergies	allergic reaction to insetct sting	Base44		24 44 24 21				0 white		2	1
19	Allergies	allergic reaction to insetct sting	Base44		14 33 23 43				0 violet		11	1
20	Dark forces	astral attack	Base10		9999				0 yellow		10	1
21	Dark forces	astral attack	Base10		9434				0 yellow		6	1
22	Dark forces	astral attack	Base10		100777				0 red		4	1
23	Dark forces	astral attack	Base44		07 22 15 22				0 red		5	2
24	Dark forces	astral attack	Base44		34 34 44 23				0 red		3	2
25	Dark forces	overshadowing entities	Base 44		12 14 40 41				0 yellow		1	1
26	Dark forces	overshadowing entities	Base44		16 44 12 11				0 violet		4	1

The Disease Category is in first column, while the specific disease is named in second column. Each recipe can have multiple lines for treatments, which will be taken into the broadcast list when selected in the VRI4. The individual broadcasts are same like for general broadcasts and have the same rules. Required are at least Base and Rate.

You can add or change the list according to your needs and then store it again as \*.csv file. Then upload the new Recipe file. The file is stored in browser cache. It will be erased again when browser cache is erased, so please keep a backup or your recipe file.

**Table of Broadcasts**

In the table below the lines you can browse through the broadcasts, which are stored in the internal broadcast list. You can delete lines if required or simply check whether e.g. the upload or a created broadcast list was successful.

For editing the list, you need to download the broadcast list and edit it in an external spreadsheet program. Then delete the broadcast list in the VRI4 and upload your edited broadcast list again.

## Analysis – Mode

This mode wants to help you to structure and standardise and initial dowsing routine to get an overview on the situation of your client.

Usually you dowse through subtle bodies and organs to get an initial impression of the status, and then will go on with more specific questions, handling the actual situation of your client.

The Analysis mode will help you with the standardised part of the dowsing, presenting you a sequence of rates to dowse for. This sequence can be taken from a template or you can create your own sequence and upload it into the instrument. After having performed the dowsing, you can download the list including the results to put it into your documentation for later reference, and to create potential broadcasts out of them.



### How to

Make sure you have already included the name and/or the picture of your client in the instrument (HOME or SETTINGS page). If you want to use the speech functions, you need to select language and a speaker on the Settings page. Language and Speaker selection are depending on what you have got installed on your PC or tablet and are not part of the VRI4.

Select a name  
Adam Cooper

HOME

Organs

Auditory

Deviation

ADD TO LIST

START

SKIP

CONT

FLIP CHARTS

RESULT

INTERIOR

TEMPLATE

TEMPLATE

CLEAR LIST

Keyboard
  Speech

Sorter	Name	Base	Rate	Category	Topic	Question	Target	Result
0	Adam Cooper	10	40.8	Miasm	Psora Miasm	Degree	100r	🗑️
1	Adam Cooper	10	914508	Organs	Auditory	Deviation	100r	🗑️

Rows per page: 10 | 1-2 of 2 | < >

## General use and workflow of Analysis Mode

The VRI4 supports dowsing routines and facilitates the documentation of your dowsing results. With uploading your own dowsing routines, you can adapt the VRI4 Analysis mode according to your personal preferences.

The VRI4 has an internally built in template which supports the standard dowsing routines you usually use with initial Analysis. Available dowsing questions can be selected with the three drop boxes above the scale.

### The general Workflow would be as following

- 1.) Select or upload the dowsing categories or questions you want to dowse for and add those to the list
- 2.) Start the dowsing process. The dowsing questions are presented and you can input your dowsing requests via screen touch (tablets) or with keyboard input (PC) (for keyboard input you need to select the Keyboard switch button)
- 3.) After having completed the dowsing, you can download the results and process those outside the VRI4 (e.g. in Excel, OpenOffice or similar program) and/or add the results to your documentation.

### Details of Analysis Screen

The screenshot displays the VRI4 Analysis Mode interface. At the top, a dropdown menu (1) shows the user's name 'Grace Howard' and a 'HOME' button. Below this, two more dropdown menus (2) show 'Subtle Anatomy' and '..all..'. A central semi-circular scale (4) is used for dowsing, with a needle pointing to approximately 10%. The scale is divided into 'understimulation / congestion' (red) and 'overstimulation' (green) zones. To the right of the scale are buttons for 'START' (4), 'SKIP', and 'CONT'. Below the scale are buttons for 'RESULT' (5), 'TEMPLATE' (6), and another 'TEMPLATE' button. On the left side, there are buttons for 'FLIP CHARTS' (9), 'INTERIOR' (10), and 'CLEAR LIST' (11). At the bottom right, there are checkboxes for 'Keyboard' (7) and 'Speech' (8). A central image of 'Grace Howard' is overlaid on the scale. At the bottom, a table (3) displays the dowsing results.

Sorter	Name	Base	Rate	Category	Topic	Question	Target	Result
0	Grace Howard	10	2935	Subtle Anatomy	Etheric Body	Congestion / Overstimulation	-100	
1	Grace Howard	10	2935	Subtle Anatomy	Etheric Body	Abberation	100r	
2	Grace Howard	10	9027	Subtle Anatomy	Astral Body	Congestion / Overstimulation	-100	
3	Grace Howard	10	9027	Subtle Anatomy	Astral Body	Abberation	100r	

Rows per page: 25 1-4 of 4

- 1.) Drop down box to select the client. The name and picture of the selected client is displayed as witness for dowsing. You need to have set the client name in beforehand in either Settings or Ratebook screen!
- 2.) 3 Drop down boxes where you can select the topic you want to dowse for. These entries are coming either from the template which is built in or from the template you have uploaded to the VRI4. With "Add to list" this entry will be pushed down to the dowsing list (3). When you select ...all., all entries of the corresponding list will be added.
- 3.) Dowsing list. In this list the entries are collected which have been added as described before. You can delete a row with the red button on the left and you can delete a result with the blue button on the right side.
- 4.) With START you can start the dowsing procedure. The VRI4 will display the first question on the upper left side of the dowsing chart. You can input your result for this dowsing question by touching the scale on the screen at the appropriate position (with tablets) or by keyboard input (PC). For Keyboard input you need to switch Keyboard switch on (8). In case your computer supports speech output, you can switch 'Speech' on. If a system or installed language voice is available, the computer will read the dowsing question aloud.
- 5.) After finishing the dowsing procedure, you can download the filled list with the "Result" button.
- 6.) You can create you own template and upload it with the Template upload button (violet button). You can download the currently used template with the download button (green button). The files are comma delimited csv files, which can be read and modified with a variety of programs e.g. Excel, OpenOffice or other.
- 7.) Input field for keyboard input. This is automatically activated when switching on Keyboard (8). Because with tablets, the virtual keyboard will be shown on the screen, you may not switch on the keyboard in tablet computers. With PC you can simply type the dowsed numbers and press Enter to go to the next dowsing question.
- 8.) Keyboard – see above. Speech – switch this on, when your computer is capable to generate speech from text. You can select the language and voice in the Settings page.
- 9.) You can flip the charts between a red and green 0-100% and a -100 to +100% Chart.
- 10.)This button allows you the check the interior setting of the dials for dowsing
- 11.)This will clear the dowsing list on the bottom, so you can start over with creation of a new list.

## Description of the Analysis template file (comma delimited CSV file)

Sorter	Base	Rate	Category	Topic	Question	Target	Result
1	10	10	2935 Subtle Anatomy	Etheric Body	Congestion / Overstimulation	-100	
2	10	10	2935 Subtle Anatomy	Etheric Body	Abberation	100r	
3	10	10	9027 Subtle Anatomy	Astral Body	Congestion , with or without, Overstimulation	100r	
4	10	10	9027 Subtle Anatomy	Astral Body	Abberation	100r	
5	10	10	1047 Subtle Anatomy	Mental Body	Congestion / Overstimulation	100r	
6	10	10	1047 Subtle Anatomy	Mental Body	Abberation	100r	
7	10	10	669755 Subtle Anatomy	Nadis	Congestion / Overstimulation	100r	
8	10	10	669755 Subtle Anatomy	Nadis	Abberation	100r	
9	10	10	10.9 Subtle Anatomy	Aura	Congestion / Overstimulation	100r	
10	10	10	3317 Subtle Anatomy	Lack of Coordination Phys.-Etheric	Degree	100r	
11	10	10	2710.11 Subtle Anatomy	Lack of Coordination Etheric-Astral	Degree	100r	
12	10	10	31719 Subtle Anatomy	Lack of Coordination Astral -Mental	Degree	100r	
13	10	10	40.8 Miasm	Psora Miasm	Degree	100r	
14	10	10	70.4759 Miasm	Syccosis Miasm	Degree	100r	
15	10	10	50.908 Miasm	Syphilis Miasm	Degree	100r	
16	10	10	40.288 Miasm	Tuberculosis Miasm	Degree	100r	
17	10	10	60.749 Miasm	Cancer Miasm	Degree	100r	

Sorter – only for an initial enumeration

Base – Rate Base for the Rate you are giving in the next column. Allowed are 10, 44 and 336.

Rate – Radionic rate used for analysis dowsing

Category – displayed in the first drop down list as the upper most structure criteria of your list

Topic – displayed in the second drop down list as the more detailed criteria.

Question – This text is related to the rate given in the line and will be, together with the topic, displayed and read loud for dowsing. This text can be adapted to your needs.

Target – this column determines the scale which is used for dowsing. 100r and 100g means a 0-100% scale with either red or green background. -100 will display a -100to100% scale.

Result – is empty in the template. After dowsing and download of the template, this column is filled with the results of your dowsing run.



P.S.

Because the VRI4 is still in programming, you may encounter some errors. I have tried to test all functions, however may not have covered all possibilities which may cause errors or unexpected behaviors. Please send me an email if you encounter any problems, so I can update the VRI4 accordingly. Email contact: [Geoffrey.Ardens@gmail.com](mailto:Geoffrey.Ardens@gmail.com)

The 4.1 Version including the analysis mode can be downloaded at <https://virtual-radionics/VRI4>.

The older version v4.0 can still be downloaded from Microsoft Azure (<https://brave-glacier-087932403.5.azurestaticapps.net/>).

With time I will try to build an FAQ page, based on frequently asked questions if required.